


## LINEARITY

The narrow line width and large reduction in non resonance spectra provides the analyst with an almost linear calibration curve. This means for most determinations only one standard is required for calibration.

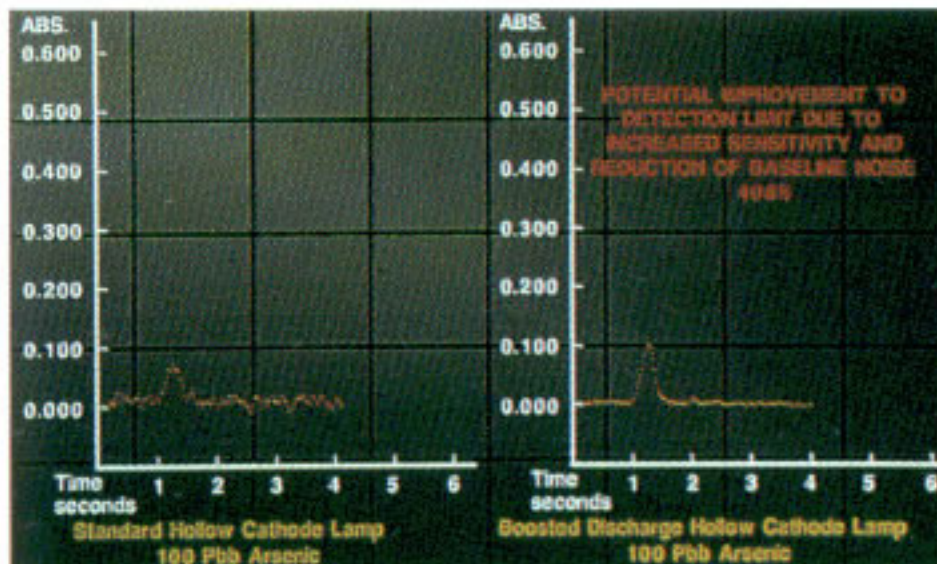

## THE RESULT

The comparison of a hollow cathode lamp and a Super Lamp for a furnace determination of Arsenic clearly illustrates the performance achieved.

